

TSP Calibration, Inc.

1110 S. FM 1788 Suite 38 Midland, TX 79706
 Phone: (432) 296-4992 Email: Chad@tspndt.com

Certificate of Calibration

Certificate No TSPW-05162025-008

Gage ID PEA-22261 Gage S/N 22261 Description UT Thickness Gauge Operating Procedure: OP-121 Unit of Meas. inch Manufacturer Dakota Cal. Date 5/16/2025 Next Due 11/16/2025 Cal. Freq. 6.00 Months Location Lab	Environmental Conditions Temperature 68 Deg F +/- 2 Humidity 35-55% Approved Yes Customer Info. Peak NDT Solutions
---	---

Certification Statement

TSP Calibration, Inc. calibration systems complies with the requirements of ISO 9001:2015. The equipment that is certified by this certificate has been calibrated by standards that have accuracy which is traceable to standards of the National Institute of Standards and Technology.

Findings

SO 14313 Job 14161

Standard ID	.100 "	Uncertainty		Units		Type	V
Limited Use?	No	Minimum	0.098	Nominal	0.100	Maximum	0.102
Ref Type	5 Step Block	As Found	0.100	Accuracy	0.000	Fail Before	No
		As Left	0.100	Accuracy	0.000	Fail After	No
Gage ID of Standard	REF-337214						
Std Due Date	8/8/2025	Gage S/N	337214	NIST No.	154782		
Standard ID	.200 "	Uncertainty		Units		Type	V
Limited Use?	No	Minimum	0.198	Nominal	0.200	Maximum	0.202
Ref Type	5 Step Block	As Found	0.200	Accuracy	0.000	Fail Before	No
		As Left	0.200	Accuracy	0.000	Fail After	No
Gage ID of Standard	REF-337214						
Std Due Date	8/8/2025	Gage S/N	337214	NIST No.	154782		
Standard ID	.300 "	Uncertainty		Units		Type	V
Limited Use?	No	Minimum	0.298	Nominal	0.300	Maximum	0.302

Ref Type	5 Step Block	As Found	0.300	Accuracy	0.000	Fail Before	No
		As Left	0.300	Accuracy	0.000	Fail After	No

Gage ID of Standard REF-337214
Std Due Date 8/8/2025

Gage S/N 337214 NIST No. 154782

Standard ID	.400 "	Uncertainty		Units		Type	V
Limited Use?	No	Minimum	0.398	Nominal	0.400	Maximum	0.402
Ref Type	5 Step Block	As Found	0.400	Accuracy	0.000	Fail Before	No
		As Left	0.400	Accuracy	0.000	Fail After	No

Gage ID of Standard REF-337214
Std Due Date 8/8/2025

Gage S/N 337214 NIST No. 154782


Standard ID	.500 "	Uncertainty		Units		Type	V
Limited Use?	No	Minimum	0.498	Nominal	0.500	Maximum	0.502
Ref Type	5 Step Block	As Found	0.500	Accuracy	0.000	Fail Before	No
		As Left	0.500	Accuracy	0.000	Fail After	No

Gage ID of Standard REF-337214
Std Due Date 8/8/2025

Gage S/N 337214 NIST No. 154782

Calibrated By Chad Adams

Signature

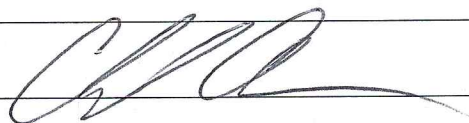

Date: 5/16/2025

APPROVED

By Kayla Myers at 4:07 pm, May 19, 2025